

JuggerKnot

SOFT ANCHOR

JuggerKnot Soft Anchor – 2.9 mm With Needles



The JuggerKnot Soft Anchor – 2.9 mm allows for guideless insertion, and is specifically designed for those who perform mini-open repairs. The rigid drill and short inserter design allows for the placement of each anchor without the need for a guide. It is loaded with either tapered or cutting needles for efficient tissue to bone attachment.



Design Features

- Guideless design allows surgeons more flexibility in placing anchors than utilizing a guide
- Pullout strength is approximately 120 lbs.¹
- Double loaded with #2 MaxBraid suture
- Tapered or cutting needle options
- Working length of inserter is 5.75 in

1. Data on file at Biomet Sports Medicine. Test Report: AT47D. Bench testing not necessarily indicative of clinical performance.


This material is intended for health care professionals and the Biomet sales force only. Distribution to any other recipient is prohibited. All content herein is protected by copyright, trademarks and other intellectual property rights owned by or licensed to Biomet Inc. or its affiliates unless otherwise indicated. This material must not be redistributed, duplicated or disclosed, in whole or in part, without the express written consent of Biomet.

Check for country product clearances and reference product specific instructions for use. For complete product information, including indications, contraindications, warnings, precautions, and potential adverse effects, see the package insert and Biomet's website.

Not for distribution in France.

BIOMET

Mini-Open Rotator Cuff Repair Using the JuggerKnot Soft Anchor – 2.9 mm with Needles and ALLthread Knotless Anchors Surgical Technique*

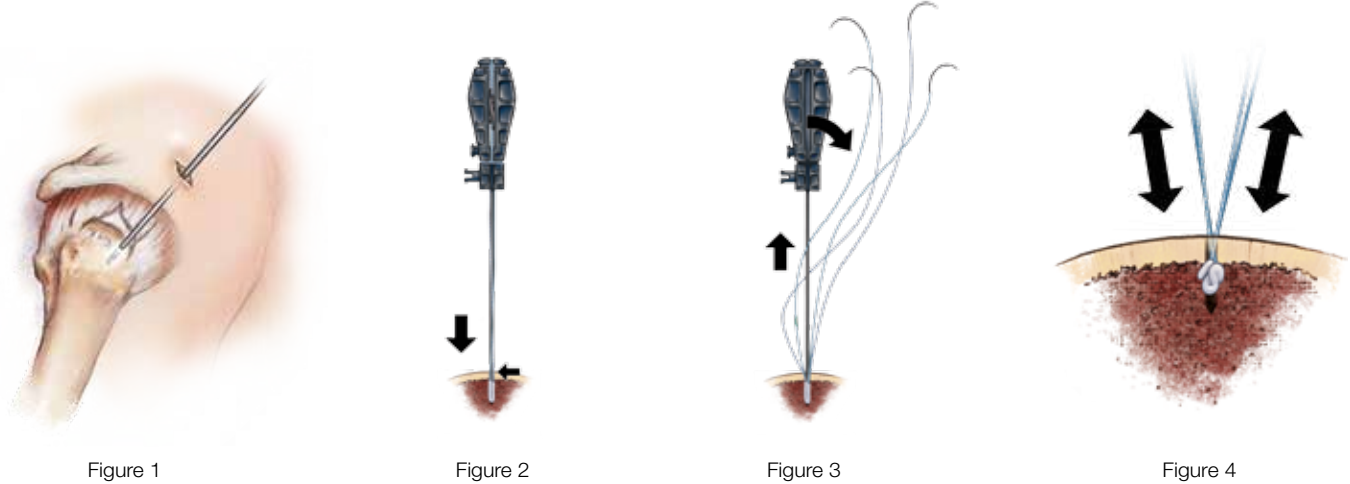

Placement of Drill

After the initial incision has been made and the tear has been assessed, visualize the bone and place the drill bit at the desired site of anchor insertion. Advance the drill until the laser etch line is even with the surface of the cortex (Figure 1). An alternate technique is to use the 2.9 mm punch; advancing the punch until the laser etch line is even with the surface of the cortex.

Insert Anchor

While maintaining the angle orientation of the drill, place the tip of the JuggerKnot Soft Anchor - 2.9 mm with needles in the freshly drilled hole (Figure 2). To advance the inserter, lightly mallet until the laser etch line is flush with the cortex.

Deploy Anchor

Pull back on the inserter to set the anchor. Carefully remove the needles from the Styrofoam inside the handle and unwrap the suture from around the handle (Figure 3). Remove the inserter by pulling straight back.

Set the Anchor

Gently pull back on all sutures until the anchor sets against the cortex. Ensure the sutures slide inside the anchor and continue with soft tissue repair per surgeon preference (Figure 4).

*Reference BMET0259.0 for full surgical technique

Part Numbers	Description
110005093	JuggerKnot Soft Anchor-2.9 mm Double Loaded #2 MaxBraid Suture with Cutting Needles
110005096	JuggerKnot Soft Anchor-2.9 mm Double Loaded #2 MaxBraid Suture with Tapered Needles
110005241	JuggerKnot Soft Anchor-2.9 mm Double Loaded #2 MaxBraid Suture with Cutting Needles 10pk
110005242	JuggerKnot Soft Anchor-2.9 mm Double Loaded #2 MaxBraid Suture with Tapered Needles 10pk
110005306	JuggerKnot Soft Anchor-2.9 mm Drill Bit Short Shaft Sterile Pack
912064	JuggerKnot Soft Anchor-2.9 mm Reusable Punch
912059	JuggerKnot Soft Anchor-2.9 mm Short Punch

BIOMET
SPORTS MEDICINE

One Surgeon. One Patient.

©2014 Biomet Sports Medicine • Form No. BMET0712.0-GBL • REV0614



Legal Manufacturer
Biomet Sports Medicine
56 East Bell Drive
P.O. Box 587
Warsaw, Indiana 46581
USA

www.biomet.com



Authorised Representative
Biomet UK Ltd.
Waterton Industrial Estate
Bridgend, South Wales
CF31 3XA
UK

CE0086