





**Compression/
Distraction Device
for Ankle Fix System,
0-15 mm
28.14.000**

Cleaning Instructions

**Set cylinder to both end positions
while cleaning with a brush.**

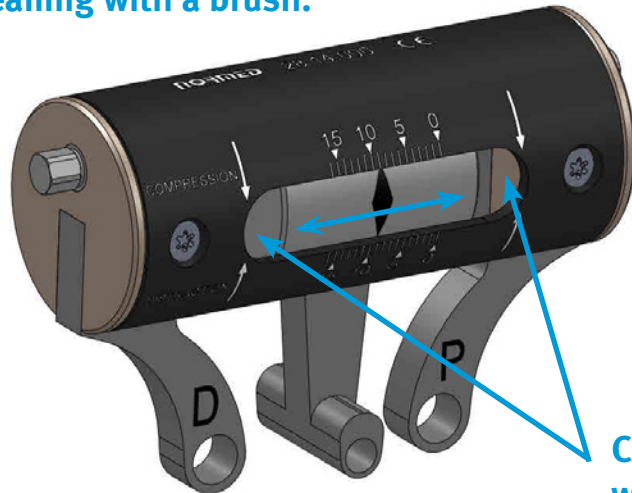

**Clean parts marked
with the arrows.**

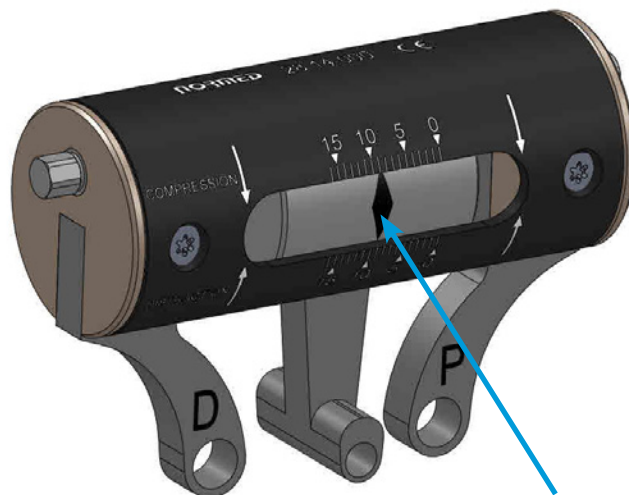

**Prior to steam sterilization, set the
cylinder in the central position.**

97-8779-094-00 ©2015 Zimmer, Inc.